

EFFECT OF LABORATORY WORKFLOW ON THE INTERNAL FIT OF PRESSED LITHIUM DISILICATE RESTORATIONS

Efecto del flujo de trabajo sobre el ajuste interno de restauraciones inyectadas de disilicato de litio

Fabian Acuña Silva,¹ Elizabeth Parra Gatica,¹ Luis Luengo,² Vilma Sanhueza,³ Ornella Contreras-Ferrada,⁴ Michael Wendler.⁵

1. Facultad de Odontología Restauradora, Universidad de Concepción, Chile.

2. Departamento de Prevención y Salud Pública, Facultad de Odontología, Universidad de Concepción, Chile.

3. Instituto de Geología Económica Aplicada (GEA), Universidad de Concepción, Chile.

4. Escuela de Salud, Instituto Virginio Gómez, Concepción, Chile.

5. Departamento de Odontología Restauradora, Facultad de Odontología, Universidad de Concepción, Chile.

ABSTRACT

Introduction: Computer-aided design and machining (CAD/CAM) and 3D printing provide interesting alternatives for fabricating patterns used in the heat-pressing technique of glass ceramics. However, there is limited evidence regarding the accuracy and precision of the resulting restorations. The aim of this study was to compare the internal fit of pressed lithium disilicate restorations produced from patterns created using manual wax-up, 3D printing, and CAD/CAM.

Materials and Methods: Thirty-six mandibular molar models with mesio-occluso-distal cavities were 3D printed. Injection patterns for these cavities were created using manual wax-up (MW), 3D printing (3DP), and CAD/CAM (CC) (n=12). Heat pressing was conducted using lithium disilicate, and the resulting restorations were adhesively cemented onto the models. The obtained samples were sectioned mesio-distally, and the internal fit between the restorations and the models was analyzed using a stereomicroscope. The results were evaluated using ANOVA and Tukey's post-hoc test (0.05).

Results: The highest fit values were observed for the CC group (135 μ m), being significantly more accurate than those of the 3DP (203 μ m) and MW (224 μ m) groups. Additionally, the CC group also achieved the highest degree of precision.

Conclusion: The fabrication technique of injection patterns is a critical factor in determining the internal fit of pressed lithium disilicate restorations. While CAD/CAM remains the most accurate and precise method, 3D printing seems to be an interesting alternative for the future.

Keywords: Prosthesis fitting; Computer-aided-design/Computer-aided-machining; 3-D printing, Lithium disilicate; Ceramics; Workflow

RESUMEN

Introducción: El uso de diseño y maquinado asistidos por computadora (CAD/CAM), así como la impresión 3D, representan alternativas interesantes para la confección de patrones para la inyección de cerámicas vítreas. Sin embargo, existe poca evidencia sobre la exactitud y precisión de las restauraciones obtenidas. El objetivo del presente trabajo es comparar el ajuste interno de restauraciones inyectadas de disilicato de litio obtenidas a partir de patrones confeccionados mediante encerado manual, impresión 3D y CAD/CAM.

Materiales y métodos: Se imprimieron 36 modelos de molares mandibulares con una cavidad mesio-occlusodistal. Se confeccionaron patrones de inyección para estas cavidades mediante encerado manual (EM), impresión 3D (I3D) y CAD/CAM (CC) (n=12). Los patrones fueron inyectados con disilicato de litio y las restauraciones cementadas adhesivamente sobre los modelos. Las muestras obtenidas fueron seccionadas mesio-distalmente y se analizó el ajuste interno entre la restauración y el modelo con una lupa estereoscópica. Los resultados fueron analizados mediante ANOVA de una vía y la prueba post-hoc de Tukey ($p=0.05$).

Resultado: El grupo CC mostró los valores más altos de ajuste (135 μ m), los que resultaron significativamente más exactos que los de los grupos I3D (203 μ m) y EM (224 μ m). CC también obtuvo los niveles más altos de precisión.

Conclusión: La técnica de confección del patrón es un factor determinante en el ajuste interno de restauraciones inyectadas de disilicato de litio. Pese a que el CAD/CAM sigue siendo la técnica más exacta y precisa, la impresión 3D aparece como una alternativa interesante de cara al futuro.

Palabras Clave: Ajuste de Prótesis; Diseño Asistido por Computadora; Impresión Tridimensional; Disilicato de litio; Cerámica; Flujo de Trabajo

CORRESPONDING AUTHOR: Michael Wendler. Roosevelt 1550, Concepción, Chile. E-mail: mwendler@udec.cl

CITE AS: Acuña-Silva F, Parra-Gatica E, Luengo L, Sanhueza V, Contreras-Ferrada O, Wendler M. Effect of laboratory workflow on the internal fit of pressed lithium disilicate restorations. *J Oral Res.* 2024; 13(1):420-430. doi:10.17126/joralres.2024.038

Received: January 14, 2024.

Accepted: May 24, 2024.

Published online: December 31, 2024

ISSN Print 0719-2460

ISSN Online 0719-2479

INTRODUCTION

Indirect glass-ceramic restorations are an essential tool in the therapeutic arsenal of the modern dentist, providing solutions for various problems, such as the loss of dental tissue caused by caries, fractures, or endodontic treatments. These materials, notable for their high resistance (over 400 MPa),¹ high translucency and aesthetics,² as well as their strong adhesive capacity,³ have extended their indication to cover the entire restorative spectrum, while maintaining an adequate balance between a minimally invasive approach and exceptional mechanical properties.^{4,5}

The heat pressing technique was one of the most significant advances in restorative dentistry of the last century, particularly due to its simplicity and ability to customize restorations to meet patient needs.⁶ Although his technique was originally based on analogue methods (such as manual waxing of plaster models), the emergence of digital workflows, including CAD/CAM (computer-aided design – computer-aided machining), and 3D printing, has expanded the range of available alternatives.⁷ Digital designs can be used to obtain patterns for the heat pressing technique, enhancing the precision and accuracy of restorations,^{8,9} thus improving the overall efficiency of the process.

Although digital technologies seem to offer more sustainable and efficient solutions than analogue methods for the heat-pressing technique, there is currently insufficient evidence regarding their effect on the precision and accuracy of these

restorations. Therefore, the aim of this research was to compare the internal fit of pressed lithium disilicate restorations obtained from patterns fabricated by manual waxing, 3D printing, and CAD/CAM. The working hypothesis was that the internal fit of pressed lithium disilicate restorations depends on the injection pattern fabrication technique.


MATERIALS AND METHODS

An *in vitro* experimental study was conducted. A mandibular second molar with a mesio-occluso-distal (MOD) cavity, with occlusal and axial depths of 3 mm, was designed using ExoCAD (v.3.1, DentalCAD, Rijeka, Germany), (Figure 1).

From this digital design, thirty-six 3D models were printed using Aquagray resin (Phrozen, Taiwan). After alcohol and water, the models underwent photopolymerization in a UW-01 oven (Creality, Shenzhen, China), following manufacturer's instructions.

Figure 1.

Digital design of a mandibular molar with a MOD cavity.

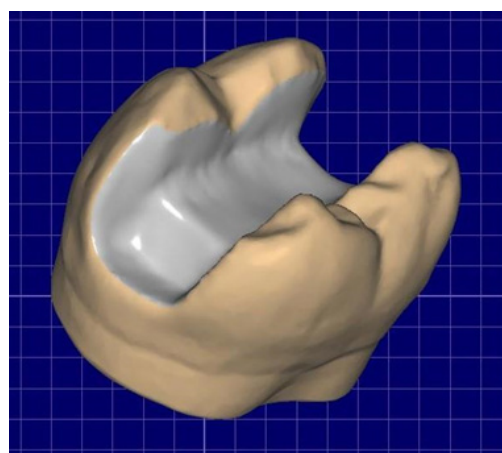

The resulting models were randomly assigned to one of the following groups (n=12) for the preparation of the injection patterns:

- Manual wax-up (MW): Wax patterns (Schuler Dental, Germany) were contoured by a single dental technician using the wax-up technique (Figure 2A). All patterns were made by the same technician.
- CAD/CAM (CC): MOD restorations were digitally designed (Figure 2B) and the injection patterns were subsequently milled from a castable wax disk (Harvest dental, Columbia, United States).
- 3D printing (3DP): Using the same digital designs as in group CC, injection patterns were 3D printed using a castable 3D resin (Prizma Marketch Labs., Brazil), as shown in Figure 2C. The obtained patterns were washed in alcohol and water, and then polymerized in the UW-01 oven.

Injection sprues were attached to the resulting patterns and then positioned in the investment ring. Following setting of the investment material, dewaxing was conducted at 850°C. The rings were then heat-pressed at 930°C using lithium


disilicate (Mazic Press, Vericom, Korea), in a Vacumaat furnace (Vita Zahnfabrik, Bad Säckingen, Germany).

Once removed from the investment rings, the restorations were washed with a solution of 0.6% hydrofluoric acid and 1.7% sulfuric acid to remove the reactive layer. The restorations were then adhesively cemented onto the printed resin models using the following protocol:

1. The printed models were cleaned with 96% ethanol.
2. The restorations were conditioned with 10% hydrofluoric acid (Condac Porcelana, FGM, Brazil) for 20 seconds.
3. Ultrasonic washing of the etched restorations was conducted in a 96% ethanol bath for 5 minutes.
4. Two layers of silane (Prosil, FGM, Brazil) were applied.
5. Dual resin cement (U200, 3M, St. Paul, MN, United States) was applied to the inner surface of the restoration, and finger pressure was used for cementation.
6. Excess cement was removed with a microbrush.
7. After two minutes of waiting setting, the restorations were light-cured for 30 s using a Bluephase N photocuring unit

Figure 2.


Fabrication techniques for the injection patterns.

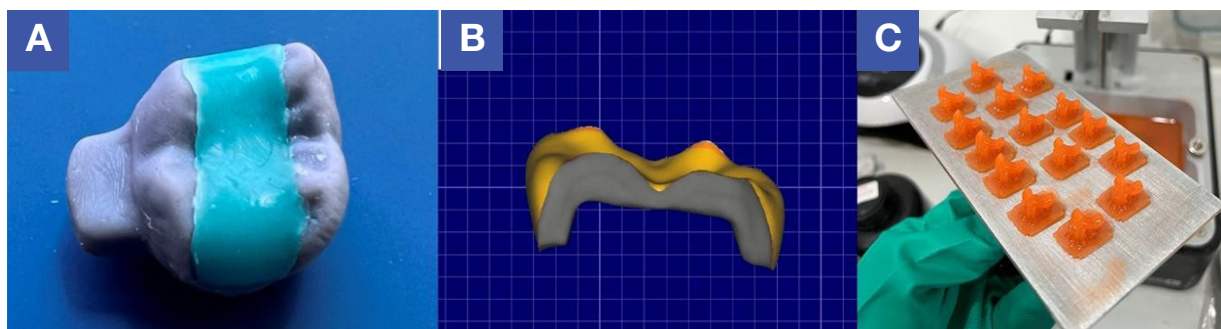

A: Manual waxing. **B:** CAD-CAM milling. **C:** 3D-Printing.

Figure 3.

Mesio-distal section of a sample indicating the location of the 8 measurement points for internal fitting (A-H).

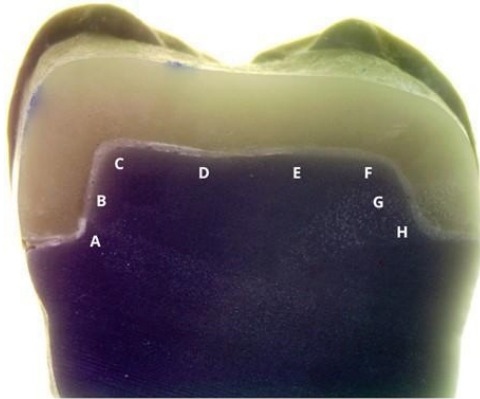

(Ivoclar-Vivadent, Schaan, Liechtenstein) at 1200 mW/cm². Obtained samples were stored in a dry environment for 24 hours to ensure complete polymerization of the cement and were subsequently sectioned mesio-distally using a precision saw (IsoMet 1000, Buehler, USA) equipped with a diamond blade under continuous cooling.

Obtained sections were then analyzed with a stereomicroscope (SF-TRA, Am-Scope, United Scope LLC, Irvine, CA, USA) at 20x magnification. The internal fit was assessed by measuring the thickness of the cement layer at eight internal locations, designated with the letters A to H, (Figure 3).

All measurements were performed by the same observer, who was blinded to the fabrication technique used in each case. Additionally, one sample per group was prepared for scanning electron microscopy (SEM) analysis, and micrographs of the restoration-cement-model interface were obtained (TES-CAN VEGA II LSH, TESCAN ORSAY HOLDING a.s., Brno, Czech Republic).

The internal adjustment results were analyzed using bivariate descriptive statistics. A one-way analysis of variance (ANOVA) was conducted to test the working hypothesis. Multiple comparisons between groups were

Figure 4.

Distribution and standard deviation of the internal fit data for each group at each measurement location. The dotted line indicates an ideal reference value for internal fitting, set at 120 µm.

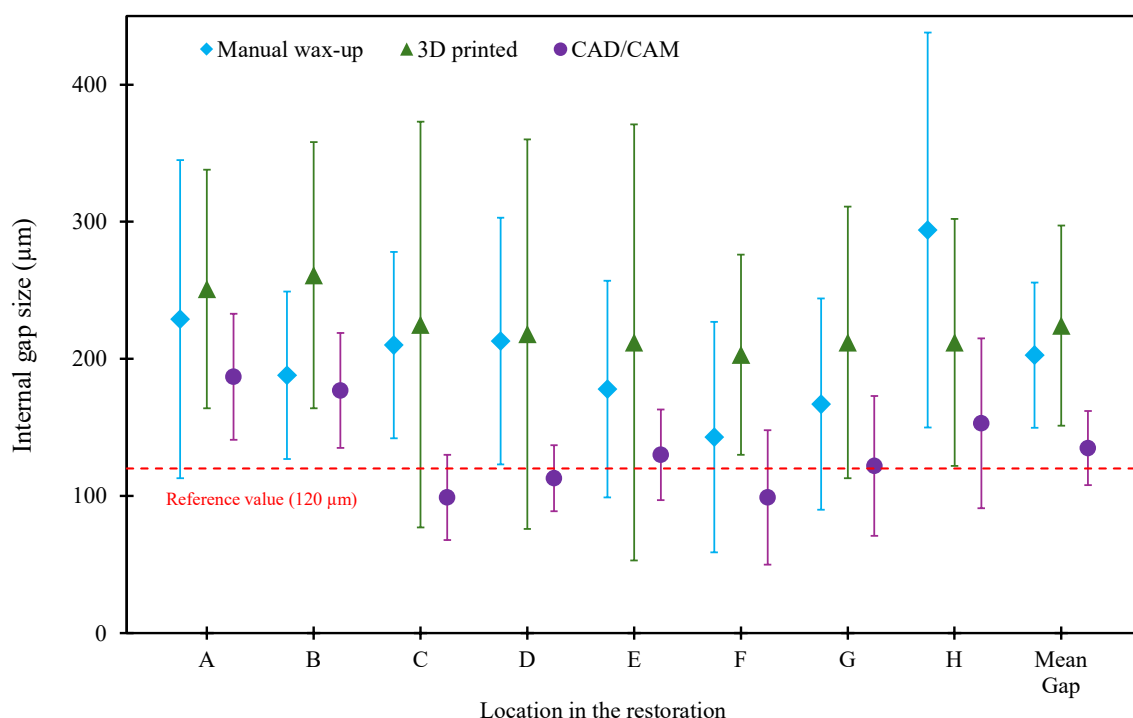


Figure 5.

Micrography of the internal fit of a restoration from the 3DP group. The insets show variations in the thicknesses of the cement layer (cem), proving that the fit level of the ceramic restoration (cer) is not uniform along the interface. Magnification of the general view: 72X. Magnification of the insets: 312X.

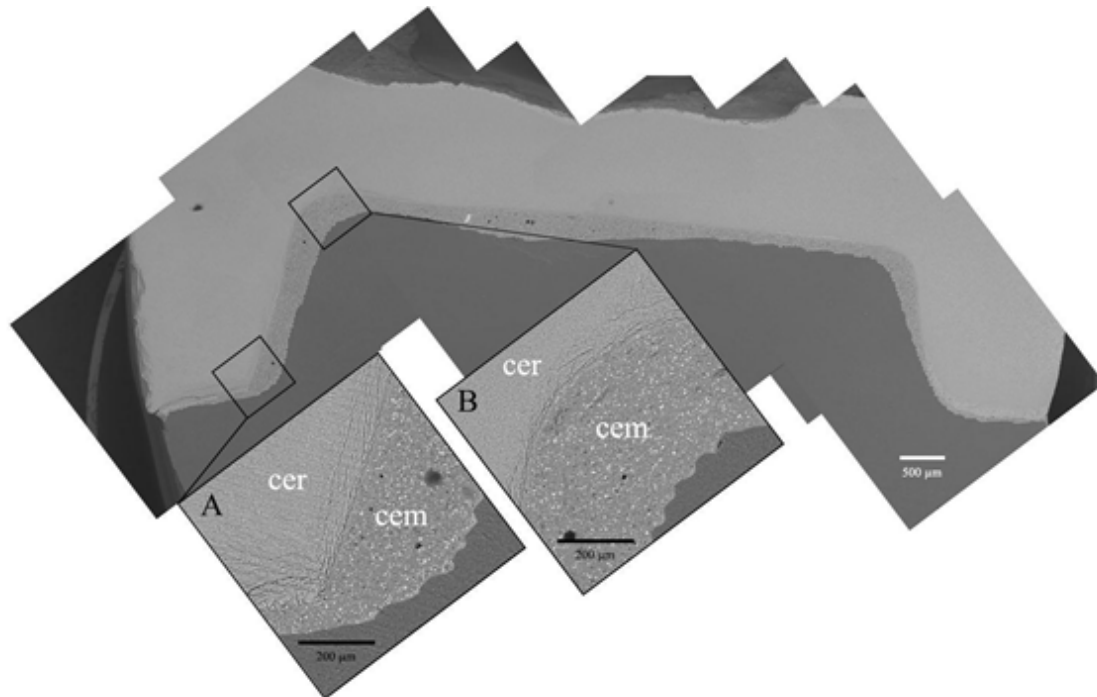


Table 1

Mean values of the internal gap (μm) of the restorations at each of the measured points, with their respective standard deviations (in parenthesis).

Point	Manual waxing	3D printing	CAD/CAM
A	229 (116) ^A	251 (87) ^A	187 (46) ^A
B	188 (61) ^A	261 (97) ^B	177 (42) ^A
C	210 (68) ^B	225 (148) ^B	99 (31) ^A
D	213 (90) ^B	218 (142) ^B	113 (24) ^A
E	178 (79) ^A	212(159) ^A	130 (33) ^A
F	143 (84) ^{A,B}	203 (73) ^B	99 (49) ^A
G	167 (77) ^{A,B}	212 (99) ^B	122 (51) ^A
H	294 (144) ^B	212 (90) ^{A,B}	153 (62) ^A
Mean	203 (53) ^B	224 (73) ^B	135 (27) ^A

Mean values followed by the same superscript letter in each row are not statistically different.

performed using Tukey's post hoc test with a confidence level of 5%. Statistical analyses were carried out using SPSS-27 software.

RESULTS

The results obtained for internal fit are presented in Table 1. The mean fit value of the CC group (135 μm) was significantly lower than that of the MW (203 μm) and 3DP (224 μm) groups, which did not differ significantly from each other.

At the internal level, no statistically significant differences were observed between the three groups at points A and E, while the largest differences were found at points C and F. Most of the values of the MW group were statistically comparable to those of the 3DP group.

The distribution of the internal fit along the restoration-model interface is shown in Figure 4. Using a minimum fit value of 120 μm as a reference, it is clear the CC group consistently exhibits greater accuracy than the MW and 3DP groups.

In addition, the lower standard deviations in this group also highlight its greater precision. Figure 5 shows a micrograph of a sample from the 3DP group, highlighting the inhomogeneity in the thickness of the cement layer. It is interesting to note that, in the peripheral areas of the restoration, the final fit is better than in the internal areas, as illustrated in the insets.

DISCUSSION

New technologies, such as CAD/CAM and 3D printing, are playing a crucial role in modern dentistry, revolutionizing traditional approaches to the fabrication of indirect restorations. The rapid evolution of these technologies has created an innovative landscape, providing not only greater efficiency, but also enhanced precision and customization in dental treatments.⁷ The results of this study partially confirm this trend, revealing a clear difference in both the accuracy and precision of digital versus analog techniques in the fabrication of wax patterns for the injection of glass ceramics.

Consequently, the initial hypothesis is confirmed, as the method of pattern fabrication had a significant effect on the internal fit of the resulting restorations. One of the main challenges when studying the fit of indirect restorations is the lack of consensus regarding the ideal value of internal fit. In this study, a minimum acceptable value of 120 μm was established, a magnitude supported by various studies in the literature.¹⁰⁻¹² In this regard, the best results were observed in the CC group, which had an average fit of 135 μm across the 8 analyzed locations, being therefore the closest to the ideal value. In contrast, the MW and 3DP groups recorded values of 224 μm and 203 μm , respectively, distancing themselves from what would be defined as clinically acceptable based on this criterion.

There are few studies in the literature comparing the fit of restorations obtai-

ned using differently fabricated injection patterns, especially those obtained using digital technologies.⁶ In the study by Guachetá *et al.*,⁹ injected lithium disilicate veneers made from a digital design and printed in castable resin were compared with veneers made using manual waxing. Although the digital model group had a smaller internal gap than the waxed samples (61.21 μm versus 68.03 μm), these differences were not statistically significant.

In another study by Ottoni *et al.*,⁸ crowns made from 3D-printed patterns were compared with those obtained using the milled pattern technique. The internal fit obtained using micro-computed tomography showed similar outcomes for both groups, suggesting comparable accuracy between the two techniques. On the other hand, using an experimental design, very similar to the one adopted in the present study, Homsy *et al.*,¹³ found that, for pressed restorations (IPS e.max Press), the best marginal and internal fits were obtained from subtractively manufactured wax patterns (CAD-CAM), compared with patterns produced by manual waxing or 3D printing. As in the present study, no differences were observed between the two additive techniques.

The larger mismatch observed here in restorations obtained using the 3D printing technique could be explained by factors such as the software used for the design,¹⁴ the number of layers configured for the final print, the arrangement of the supports adhered to the printing base,¹⁵ the printing speed,¹⁶ the contraction

inherent to this type of material,¹⁷ and the post-processing in alcohol once the print was completed and removed.¹⁵ On the other hand, the lower accuracy observed in the manual waxing technique can be attributed to the negative effects of the thermal sensitivity of the patterns, which, when subjected to heat during casting, can experience a higher thermal expansion, potentially altering their dimensions.¹⁸

Another relevant factor is that the handling of the patterns is directly linked to the skills and knowledge of the dental laboratory technician.^{13,18,19} The higher accuracy and precision of the CC group could be explained by the lesser influence of the human factor, as the patterns were obtained systematically through machining. In addition to the more detailed and faithful reproduction of the dental anatomy, this technique ensures a higher precision of the restorations,²⁰ in an efficient and faster manner,^{21,22} thus, significantly reducing working times.

Although the restorations in the 3DP group were not statistically more accurate than those in the MW group, a slight trend towards better internal adaptation was observed (Table 1). This technique is still relatively new, so it faces challenges inherent to its development and is dependent upon several factors that may have contributed to errors in the manufacturing process.¹⁴⁻¹⁷ Improving the quality of 3D-printed patterns, therefore, requires a full understanding of these factors to improve their accuracy and consistency.²³

One of the limitations of this work was

the use of 3D-printed tooth models. Although this approach is innovative and allows for the creation of identical cavities for cementation of restorations, its use prevents a direct comparison with studies carried out on real teeth, especially regarding the adhesive fixation of restorations. However, by isolating the precision factor in cavity preparation, it is possible to better analyze the effect of the manufacturing technique on the accuracy of the resulting patterns.

The findings of this study confirm the leadership of CAD/CAM technology in the digital transformation process. However, 3D printing represents an increasingly efficient alternative, both in terms of time and cost. It is therefore essential to continue researching and investing in this technology,, whose contribution to dentistry, both present and future, is promising.

CONCLUSION

The laboratory workflow is a determining factor of the internal fit of injected/pressed lithium disilicate restorations, with the CAD/CAM technique achieving levels of fit and precision not only approaching the ideal of 120 µm, but also significantly surpassing those of manual waxing and 3D printing techniques.

Although 3D printing seems to be a more efficient and innovative solution, its development still requires improvements in several factors that currently influence its performance.

CONFLICT OF INTERESTS

The authors declare that they have no conflict of interests.

ETHICS APPROVAL

The work reported in this paper did not include work on humans, animals or tissues derived from these. Therefore, bioethics approval was not required for its execution.

FUNDING

This work was carried out with funds from the Master's program in Dental Sciences of the Faculty of Dentistry of the University of Concepción.

AUTHORS' CONTRIBUTIONS

Fabián Acuña: Conceptualization, methodological design and execution, analysis of the results and writing of the manuscript.

Elizabeth Parra: Methodological execution and analysis of the results.

Luis Luengo: Analysis of the results.

Vilma Sanhueza: Methodological execution.

Ornella Contreras-Ferrada: Methodological execution.

Michael Wendler: Conceptualization, methodological design, review of the manuscript.

ACKNOWLEDGEMENTS

None.

ORCID

Fabian Acuña Silva

 0009-0006-3099-9160

Elizabeth Parra Gatica

 0000-0001-7285-015X

Luis Luengo

 0000-0002-9643-4334

Vilma Sanhueza

 0000-0002-6874-2428

Ornella Contreras-Ferrada

 0009-0006-4360-4455

Michael Wendler

 0000-0002-6899-6591

PUBLISHER'S NOTE

All statements expressed in this article are those of the authors alone and do not necessarily represent those of the publisher, editors, and reviewers.

COPYRIGHT

This is an open-access article distributed under the terms of the [Creative Commons Attribution License \(CC BY 4.0\)](https://creativecommons.org/licenses/by/4.0/). The use, distribution or reproduction in other forums is permitted, provided the original author(s) and the copyright owner(s) are credited and that the original publication in this journal is cited, in accordance with accepted academic practice. No use, distribution or reproduction is permitted which does not comply with these terms. © 2024.



PEER REVIEW

This manuscript was evaluated by the editors of the journal and reviewed by at least two peers in a double-blind process.

PLAGIARISM SOFTWARE

This manuscript was analyzed Compilatio plagiarism detector software. Analysis report of document ID.13047ea74688a045fb032bc9746b947b2b9f4dc4

ISSN Print 0719-2460 - ISSN Online 0719-2479.

<https://www.joralres.com/index.php/JOralRes/issue/archive>

REFERENCES

1. Wendler M, Belli R, Petschelt A, Mevec D, Harrer W, Lube T, Danzer R, Lohbauer U. Chairside CAD/CAM materials. Part 2: Flexural strength testing. *Dent Mater.* 2017 Jan;33(1):99-109. doi: 10.1016/j.dental.2016.10.008. Epub 2016 Nov 21. PMID: 27884403.
2. Wang F, Takahashi H, Iwasaki N. Translucency of dental ceramics with different thicknesses. *J Prosthet Dent.* 2013 Jul;110(1):14-20. doi: 10.1016/S0022-3913(13)60333-9. PMID: 23849609.
3. Monteiro RS, Ferrairo BM, José de Azevedo-Silva L, Minim PR, Rubo JH, Furuse AY, Silikas N, Sanches Borges AF. Glass ceramics behave like selectively etched enamel on interfaces produced with self-adhesive/ self-curing resin cement. *Int. J. Adhes. Adhes.* 2023; 124: 103383. <https://doi.org/10.1016/j.ijadhadh.2023.103383>
4. Beier US, Dumfahrt H. Longevity of silicate ceramic restorations. *Quintessence Int.* 2014 Sep;45(8):637-44. doi: 10.3290/j.qi.a32234. PMID: 25126640.
5. Kois DE, Isvilanonda V, Chaibutry Y, Kois JC. Evaluation of fracture resistance and failure risks of posterior partial coverage restorations. *J Esthet Restor Dent.* 2013 Apr;25(2):110-22. doi: 10.1111/jerd.12018. Epub 2013 Mar 19. PMID: 23617385.
6. Revilla-León M, Olea-Vielba M, Esteso-Saiz A, Martínez-Klemm I, Özcan M. Marginal and Internal Gap of Handmade, Milled and 3D Printed Additive Manufactured Patterns for Pressed Lithium Disilicate Onlay Restorations. *Eur J Prosthodont Restor Dent.* 2018 Mar 1;26(1):31-38. doi: 10.1922/EJPRD_01733RevillaLeon08. PMID: 29461746.
7. Zarone F, Di Mauro MI, Ausiello P, Ruggiero G, Sorrentino R. Current status on lithium disilicate and zirconia: a narrative review. *BMC Oral Health.* 2019 Jul 4;19(1):134. doi: 10.1186/s12903-019-0838-x. PMID: 31272441; PMCID: PMC6610968.
8. Ottoni R, Marocho SMS, Griggs JA, Borba M. CAD/CAM versus 3D-printing/pressed lithium disilicate monolithic crowns: Adaptation and fatigue behavior. *J Dent.* 2022 Aug;123:104181. doi: 10.1016/j.jdent.2022.104181. Epub 2022 Jun 7. PMID: 35679990.
9. Guachetá L, Stevens CD, Tamayo Cardona JA, Murgueitio R. Comparison of marginal and internal fit of pressed lithium disilicate veneers fabricated via a manual waxing technique versus a 3D printed technique. *J Esthet Restor Dent.* 2022 Jun;34(4):715-720. doi: 10.1111/jerd.12675. Epub 2020 Nov 10. PMID: 33174306.
10. Kale E, Seker E, Yilmaz B, Özcelik TB. Effect of cement space on the marginal fit of CAD-CAM-fabricated monolithic zirconia crowns. *J Prosthet Dent.* 2016 Dec;116(6):890-895. doi: 10.1016/j.prosdent.2016.05.006. Epub 2016 Jul 25. PMID: 27460314.
11. Kim DY, Kim JH, Kim HY, Kim WC. Comparison and evaluation of marginal and internal gaps in cobalt-chromium alloy copings fabricated using subtractive and additive manufacturing. *J Prosthodont Res.* 2018 Jan;62(1):56-64. doi: 10.1016/j.jpor.2017.05.008. Epub 2017 Jun 26. PMID: 28663024.
12. Belser UC, MacEntee MI, Richter WA. Fit of three porcelain-fused-to-metal marginal designs in vivo: a scanning electron microscope study. *J Prosthet Dent.* 1985 Jan;53(1):24-9. doi: 10.1016/0022-3913(85)90058-7. PMID: 3882944.
13. Homsy FR, Özcan M, Khoury M, Majzoub ZAK. Comparison of fit accuracy of pressed lithium disilicate inlays fabricated from wax or resin patterns with conventional and CAD-CAM technologies. *J Prosthet Dent.* 2018 Oct;120(4):530-536. doi: 10.1016/j.prosdent.2018.04.006. Epub 2018 Jun 29. PMID: 30318049.
14. Plooi JM, Maal TJ, Haers P, Borstlap WA, Kuijpers-Jagtman AM, Bergé SJ. Digital three-dimensional image fusion processes for planning and evaluating orthodontics and orthognathic surgery. A systematic review. *Int J Oral Maxillofac Surg.* 2011 Apr;40(4):341-52. doi: 10.1016/j.ijom.2010.10.013. Epub 2010 Nov 20. PMID: 21095103.
15. Alharbi N, Osman R, Wismeijer D. Effects of build direction on the mechanical properties of 3D-printed complete coverage interim dental restorations. *J Prosthet Dent.* 2016 Jun;115(6):760-7. doi: 10.1016/j.prosdent.2015.12.002. Epub 2016 Jan 21. PMID: 26803175.
16. Braian M, Jimbo R, Wennerberg A. Production tolerance of additive manufactured polymeric objects for clinical applications. *Dent Mater.* 2016 Jul;32(7):853-61. doi: 10.1016/j.dental.2016.03.020. Epub 2016 Apr 24. PMID: 27118595.
17. Ide Y, Nayar S, Logan H, Gallagher B, Wolfaardt J. The effect of the angle of acuteness of additive manufactured models and the direction of printing on the dimensional fidelity: clinical implications. *Odontology.* 2017 Jan;105(1):108-115. doi: 10.1007/s10266-016-0239-4. Epub 2016 Mar 19. PMID: 26995273.

- 18.** Giordano R, McLaren EA. Ceramics overview: classification by microstructure and processing methods. *Compend Contin Educ Dent.* 2010 Nov-Dec;31(9):682-4, 686, 688 passim; quiz 698, 700. PMID: 21197937.
- 19.** Arora A, Yadav A, Upadhyaya V, Jain P, Verma M. Comparison of marginal and internal adaptation of copings fabricated from three different fabrication techniques: An in vitro study. *J Indian Prosthodont Soc.* 2018 Apr-Jun;18(2):102-107. doi: 10.4103/jips.jips_327_17. PMID: 29692562; PMCID: PMC5903172.
- 20.** Kapos T, Evans C. CAD/CAM technology for implant abutments, crowns, and superstructures. *Int J Oral Maxillofac Implants.* 2014;29 Suppl:117-36. doi: 10.11607/jomi.2014suppl.g2.3. PMID: 24660194.
- 21.** Anadioti E, Aquilino SA, Gratton DG, Holloway JA, Denry I, Thomas GW, Qian F. 3D and 2D marginal fit of pressed and CAD/CAM lithium disilicate crowns made from digital and conventional impressions. *J Prosthodont.* 2014 Dec;23(8):610-7. doi: 10.1111/jopr.12180. Epub 2014 Jul 3. PC MID: 24995593.
- 22.** Bhaskaran E, Azhagarasan NS, Miglani S, Ilango T, Krishna GP, Gajapathi B. Comparative Evaluation of Marginal and Internal Gap of Co-Cr Copings Fabricated from Conventional Wax Pattern, 3D Printed Resin Pattern and DMLS Tech: An In Vitro Study. *J Indian Prosthodont Soc.* 2013 Sep;13(3):189-95. doi: 10.1007/s13191-013-0283-5. Epub 2013 May 3. PMID: 24431733; PMCID: PMC3732698.
- 23.** Saleh WK, Ariffin E, Sherriff M, Bister D. Accuracy and reproducibility of linear measurements of resin, plaster, digital and printed study-models. *J Orthod.* 2015;42(4):301-6. doi: 10.1179/1465313315Y.0000000016. Epub 2015 Jul 28. PMID: 26216658.